

# Aranax<sup>®</sup>

Cervical Plating System



- › Lower profile plate minimizes soft tissue disruption
- › Increased screw angulation enhances bone purchase
- › Integrated locking mechanism helps prevent screw back-out
- › Implants are sterile packaged for product quality

# Aranax<sup>®</sup>


## Cervical Plating System

Larger graft windows for better visualization



Lower profile plate  
• 1.95mm midline profile

Enhanced integrated locking mechanism to increase resistance to screw back-out

Fixation pin holes

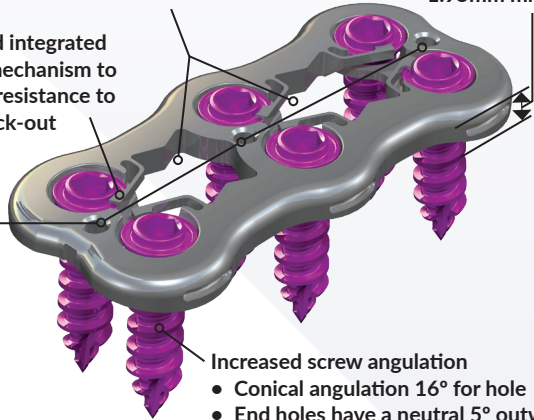


- Increased screw angulation
- Conical angulation 16° for hole
  - End holes have a neutral 5° outward angulation
  - Maximum cephalad - caudal angulation is 14°

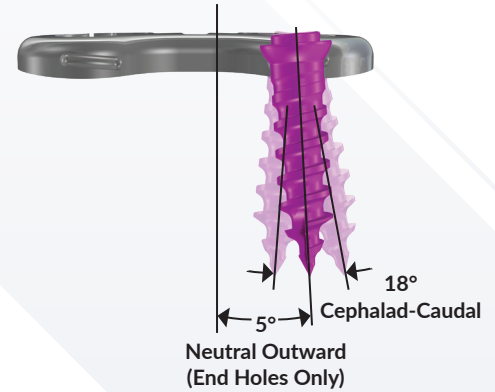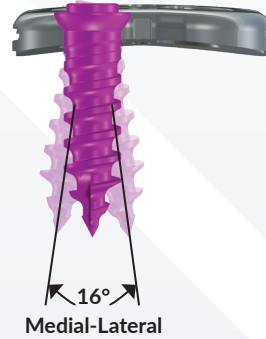

### Aranax<sup>™</sup> Plates

Item #	Levels	Screw-to-Screw Length (mm)	Total Length (mm)
X086-1009-STR	One-Level	9	20
X086-1011-STR	One-Level	11	22
X086-1013-STR	One-Level	13	24
X086-1015-STR	One-Level	15	26
X086-1017-STR	One-Level	17	28
X086-1019-STR	One-Level	19	30
X086-1021-STR	One-Level	21	32
X086-1023-STR	One-Level	23	34
X086-1125-STR	Two-Level	25	36
X086-1128-STR	Two-Level	28	39
X086-1131-STR	Two-Level	31	42
X086-1134-STR	Two-Level	34	45
X086-1137-STR	Two-Level	37	48
X086-1140-STR	Two-Level	40	51
X086-1143-STR	Two-Level	43	54
X086-1242-STR	Three-Level	42	53
X086-1245-STR	Three-Level	45	56
X086-1248-STR	Three-Level	48	59
X086-1251-STR	Three-Level	51	62
X086-1254-STR	Three-Level	54	65
X086-1257-STR	Three-Level	57	68
X086-1260-STR	Three-Level	60	71
X086-1263-STR	Three-Level	63	74
X086-1266-STR	Three-Level	66	77

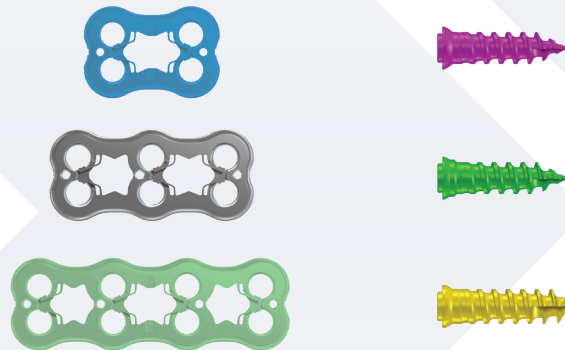

### Aranax<sup>™</sup> Screws (qty. 2/pack)

Item #	Fixed/Variable	Tip Design	Diameter (mm)	Length (mm)
X086-1412SD-STR	Variable	Self-Drilling	4.0	12
X086-1414SD-STR	Variable	Self-Drilling	4.0	14
X086-1416SD-STR	Variable	Self-Drilling	4.0	16
X086-1512ST-STR	Variable	Self-Tapping	4.25	12
X086-1514ST-STR	Variable	Self-Tapping	4.25	14
X086-1516ST-STR	Variable	Self-Tapping	4.25	16
X086-1612SD-STR	Fixed	Self-Drilling	4.0	12
X086-1614SD-STR	Fixed	Self-Drilling	4.0	14
X086-1616SD-STR	Fixed	Self-Drilling	4.0	16
X086-1712ST-STR	Fixed	Self-Tapping	4.25	12
X086-1714ST-STR	Fixed	Self-Tapping	4.25	14
X086-1716ST-STR	Fixed	Self-Tapping	4.25	16



888.886.9354  
 cs@xtantmedical.com  
 xtantmedical.com  
 664 Cruiser Ln,  
 Belgrade, MT 59714

INDICATIONS: See Package Insert for a more complete listing of indications, contraindications, warnings, precautions, and other important information.  
 LIMITED WARRANTY and DISCLAIMER: Xtant Medical products have a limited warranty against defects and workmanship and materials. Any other express or implied warranties, including warranties of merchantability or fitness, are disclaimed. WARNING: In the USA, this product has labeling limitations. See package insert for complete information. CAUTION: USA Law restricts these devices to sale by or on the order of a physician.